

## Human beta-NGF ELISA Instructions

CAT: AEH0065

### CONTENT

No.	Content	CAT. No	Volume
1	CP (Coated Plate)	EH0065CP	96 wells
2	S (Standard)	EH0065S1	9 vials
3	SD (Sample Diluent)	ESD02	12 ml/bottle
4	DA (Detect Antibody)	EH0065DA	6 ml/bottle
5	SH (Streptavidin-HRP)	ESH01	12 ml/bottle
6	AB (Assay Buffer 1×)	EAB01	12 ml/bottle
7	TS (TMB Substrate)	ETS01	12 ml/bottle
8	SS (Stop Solution)	ESS01	12 ml/bottle
9	WB (Wash Buffer 10×)	EWB01	50 ml/bottle
10	SF (Sealer Film)	ESF01	6 pieces

**NOTE:** After the kit is opened, the stabilization period of each content is 30 days, so please use the kit within 30 days after opening.


### REAGENT PREPARATION

**Washing Buffer (1×) Preparation:** Pour entire contents (50 ml) of the **Washing Buffer Concentrate** (10×) into a clean 500 ml graduated cylinder. Bring to final volume of 500 ml with glass-distilled or deionized water. Transfer to a clean wash bottle and store at 2 to 25°C.

**Standard Curve Preparation:** Reconstitute Human beta-NGF Standard by addition of distilled water as S1. Reconstitution volume is stated on the label of the standard vial. Swirl or mix gently to insure complete and homogeneous solubilization (concentration of reconstituted standard = 5000pg/ml).

Allow the standard to reconstitute for 10-30 minutes. Mix well prior to making dilutions.

Pipette 200 µl of Sample Diluent into each tube. Use the high standard to produce a 1:2 dilution series. Mix each tube thoroughly before the next transfer. Sample Diluent serves as the zero standard (0 pg/ml).

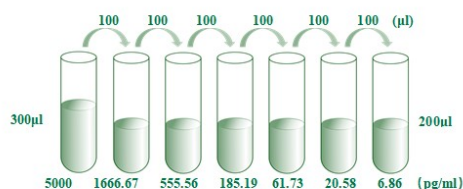


### ASSAY PROCEDURE

Bring all reagents and samples to room temperature before use.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess **CP** (Coated Plate) strips from the plate frame, return them to the foil pouch and reseal.
3. Add 50 µl of **AB** (Assay Buffer) to each well.
4. Add 50 µl or 10 µl of **Standard or sample** per well. Ensure reagent addition is uninterrupted and completed within 15 minutes.
5. Add 50 µl of **DA** (Detect Antibody) to each well.
6. Cover with an **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 1 hours on a microplate **shaker** set at 500 rpm.
7. Aspirate each well and **wash**, repeating the process four times. Wash by filling each well with WB (Washing Buffer 300 µl ). Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining WB (Washing Buffer) by aspirating or decanting. Invert the plate and **blot** it against clean paper towels.
8. Add 100 µl of **SH** (Streptavidin-HRP) to each well.
9. Cover with a new **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 30 min on a microplate **shaker** set at 500 rpm.
10. Repeat aspiration/**wash** as in step 7.
11. Add 100 µl of **TS** (TMB Substrate) to each well. Incubate for 5-30 minutes at room temperature.
12. Add 100 µl of **SS** (Stop Solution) to each well.
13. Determine the optical density within 30 minutes, using microplate **reader** set to 450 nm corrected with 570 nm or 630 nm.

**TYPICAL DATA**

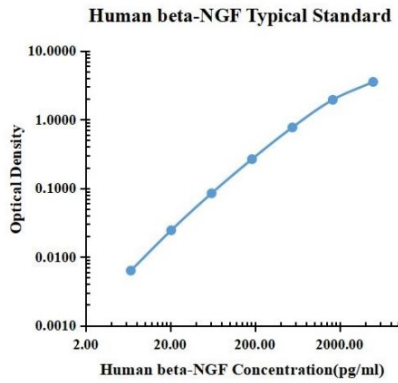

pg/ml	O.D.		Average	Corrected
0.00	0.0172	0.0164	0.0168	
6.86	0.0228	0.0234	0.0231	0.0063
20.58	0.0418	0.0405	0.0412	0.0244
61.73	0.1004	0.1016	0.1010	0.0842
185.19	0.2676	0.2957	0.2817	0.2649
555.56	0.7539	0.8159	0.7849	0.7681
1666.67	1.9450	1.9640	1.9545	1.9377
5000.00	3.3400	3.7610	3.5505	3.5337

**SENSITIVITY**

The minimum detectable dose (MDD) of human beta-NGF is typically less than 3.27 pg/ml (50 µl of sample volume) or 1.91 pg/ml (10 µl of sample volume).

The MDD was determined by adding two standard deviations to the mean optical density value of ten zero standard replicates and calculating the corresponding concentration.

**PRECISION**

- Intra-assay Precision (Precision within an assay) Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.
- Inter-assay Precision (Precision between assays).

	Intra-assay Precision			Inter-assay Precision		
	S1	S2	S3	S1	S2	S3
Sample Number	22	22	22	6	6	6
Average (pg/ml)	188.0	1692.3	2668.5	204.0	977.6	2851.8
Standard deviation	11.4	74.7	142.2	11.8	43.6	106.6
Coefficient of variation (%)	6.0	4.4	5.3	5.8	4.5	3.7

**RECOVERY**

The spike recovery was evaluated by spiking 3 levels of human beta-NGF into health human serum sample. The un-spiked serum was used as blank in this experiment.

The recovery ranged from 104% to 132% with an overall mean recovery of 117%.

**LINEARITY**

To assess the linearity of the assay, five samples were spiked with high concentration of beta-NGF in human serum and diluted with Sample Diluent to produce samples with values within the dynamic range of the assay.

The linearity ranged from 106% to 115% with an overall mean recovery of 109%.

**SAMPLE VALUES**

Serum/Plasma - Thirty samples from apparently healthy volunteers were evaluated for the presence of human beta-NGF in this assay. No medical histories were available for the donors.

Sample Matrix	Sample Evaluated	Range (pg/ml)	Detectable %	Mean of Detectable (pg/ml)
Serum	30	n.d.-17.92	87.5	7.23

n.d. = non-detectable. Samples measured below the sensitivity are considered to be non-detectable.

**DISCLAIMER AND VERSION**

For research use only. Not for use in clinical diagnostic procedures.

Copyright 2024 AREX Biosciences Ltd. Version.240820